

PNS Dual Element™

Reliable Testing of Nerve Blocker Efficacy

FEATURES




ACCURATE RESULTS

Dual Element features two snap connectors.



FLEXIBLE OPTIONS

Perforation allows electrode to be separated if desired.




1/16" AGGRESSIVE FOAM

Aggressive foam allows for superior adhesion during procedures.



NON-INVASIVE

Accurate testing of nerve block efficacy.

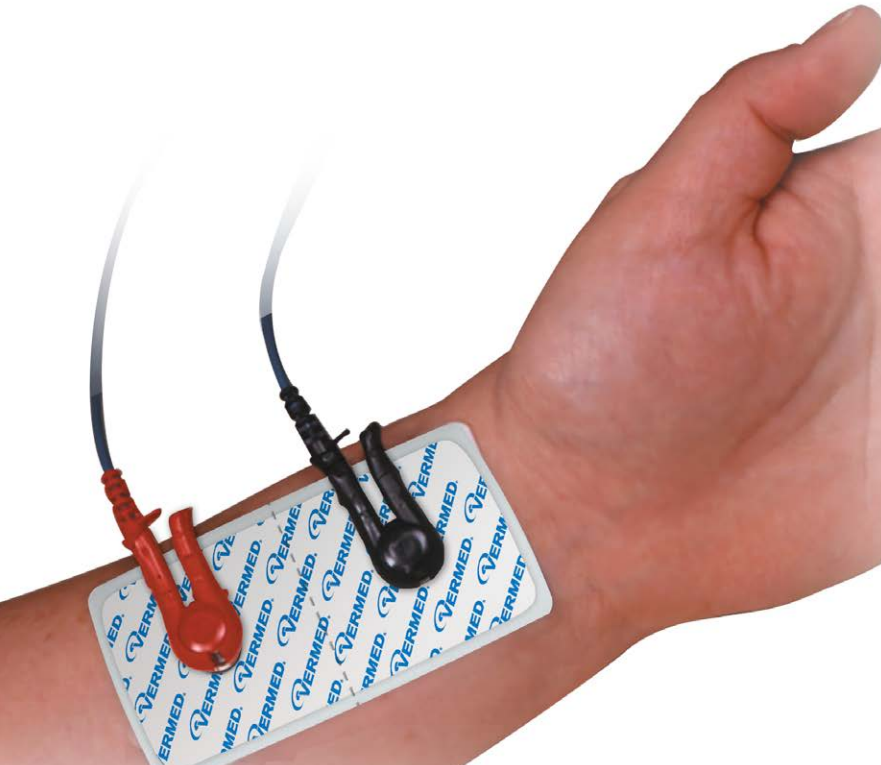

For accurate and reliable testing of nerve blocker efficacy, Vermed PNS Dual Element™ electrodes are a must.

PACKAGING

INNER BOX

Single use packs are packaged in inner boxes within the case

CASE

FDA / GS1 Compliant Labels



HYGIENIC, DISPOSABLE SINGLE-USE PACKS

Reduces risk of cross contamination of unused electrodes

1.800.669.6905 | HS.NisshaMedical.com

Patient Monitoring & Medical Surgical Consumables



PNS Dual Element™

Reliable Testing of Nerve Blocker Efficacy

For accurate and reliable testing of the effectiveness of nerve blockers, Vermed PNS Dual Element™ electrodes are a must. They are pre-gelled, disposable, and feature universal Silver / Silver Chloride snaps to provide positive stimulation. Most importantly, they are made with the same care and high standards for which all Vermed products are known.

A10011 - 3.25" x 1.625" / 82.55mm x 41.275mm - RECTANGULAR DUAL ELEMENT ELECTRODE



Product #	Ref #	Per Strip	Per Pouch	Per Box	Per Case	Wet Gel	Duration of Use
6500034V	A10011	1	1	50	300		 24 Hours

ANATOMY

A10011

Foam | Wet Gel

